

ACCELEROMETER TEST REPORT



Mfg. Lot #: _____ Model: 1521L-005 Part #: _____ Doc. Rev. -

Serial #: _____ Operator: MPC Supply Current: 4.57 mA

Calibration Date: 08/11/15 Scale Factor: 799.9 mV/G

Full Scale: 5 g SE Lot #: 15Q152Bd 0 G Bias: 6 mV

Op. Number: 120 AOP Bias: 2.40 V

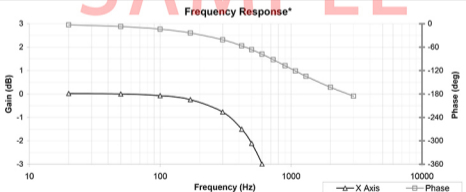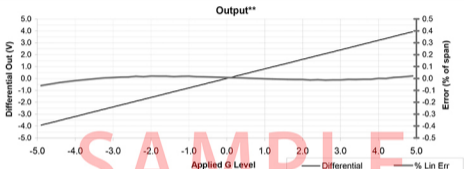

Freq. (Hz)*	20	50	100	170	300	420	500	600	730	900	1080	1300	2000	3000
dB Out - X	0.02	0.00	-0.07	-0.24	-0.77	-1.50	-2.11	-2.99	-4.28	-6.12	-8.12	-10.52	-17.16	-24.24
Phase (deg)	-2.8	-7.0	-14.0	-23.6	-41.1	-56.7	-66.5	-78.1	-91.9	-107.4	-121.1	-134.5	-162.8	-185.7

* Reference Frequency is 50 Hz

** Peak Acceleration Traceable to SDI Vibration Calibration Standard M-90152

Final Status:

Pass: